

BE PREPARED. PRESERVE LIFE.



GET TRAINED TO PRESERVE LIFE
sammedical.com


SAM[®]
MEDICAL

BLEEDING CONTROL KIT




SAM XT - INSTRUCTIONS FOR USE

STEP 1

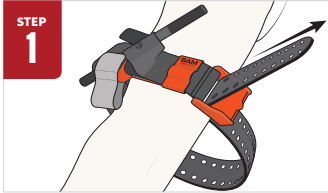


Locate the site of injury and place the **SAM® XT** around the limb, directly onto the skin 2-3 inches above the wound.

STEP 2

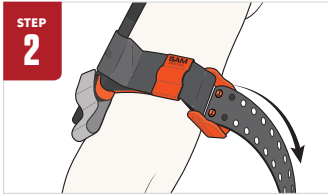


Insert the tip of the strap through the opening in the buckle. Grip the strap close to the buckle and pull hard and steady against the buckle until it stops. Maintaining tension, press the strap back upon itself to hold it in place.

STEP 3

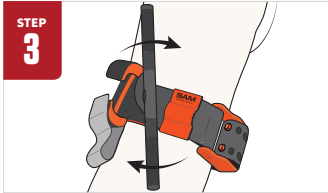


TWIST the metal windlass rod **UNTIL THE BLEEDING HAS STOPPED.**

STEP 4

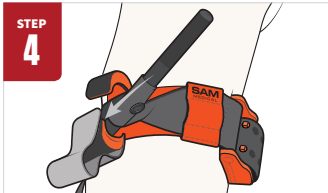

Fix the metal windlass rod inside the Windlass C-hooks and confirm that bleeding has stopped. If bleeding continues, try to further tighten the tourniquet with additional twists of the metal windlass rod. If this fails to stop the bleeding, apply a second **SAM® XT** side by side next to the first and ensure bleeding has stopped.

STEP 5

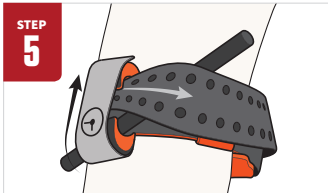


Wrap strap between Windlass C-hooks, over rod and around the limb.

Secure the (Ⓢ) Time Band over Windlass C-hooks and record time of application.

TREATMENT BY WOUND LOCATION

JUNCTIONAL INJURIES

FOR NECK, SHOULDER OR GROIN INJURIES: APPLY DIRECT PRESSURE TO THE WOUND USING THE COMPRESSED GAUZE OR PRESSURE BANDAGE

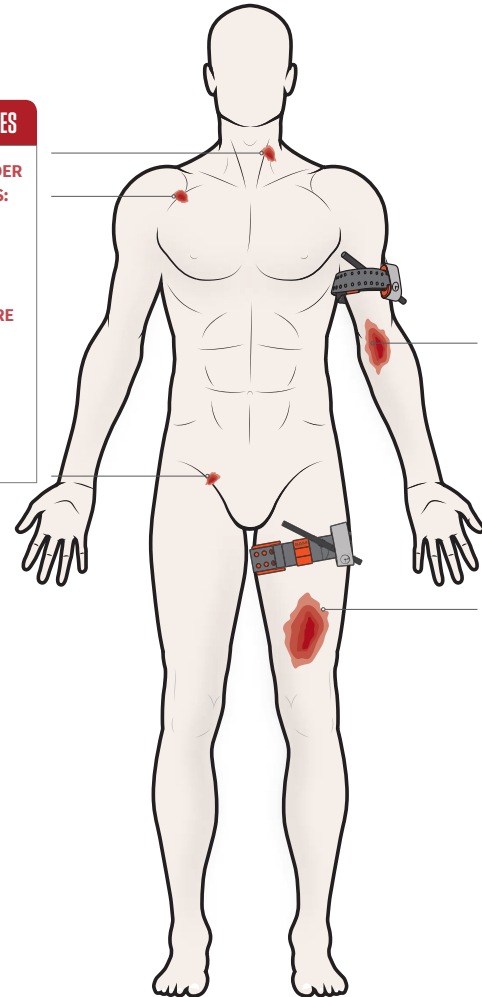

LIMB INJURIES

FOR ARM OR LEG INJURIES: APPLY THE SAM XT 2-3" ABOVE THE WOUND